



PROFICIENCY TESTING SERVICE  
AMERICAN ASSOCIATION OF BIOANALYSTS  
205 West Levee St. • Brownsville, TX 78520-5596  
800-234-5315 • 281-436-5357 • Fax 713-781-5008


**PARTIC PARTICIPANT STATISTICS**

**FIRST QUADRIMESTER 2016**

**Urine Eosinophils**

Urine Eosinophils
<b>Flagging</b>

Specimen 1	
Neg	Pos
0	12
***	

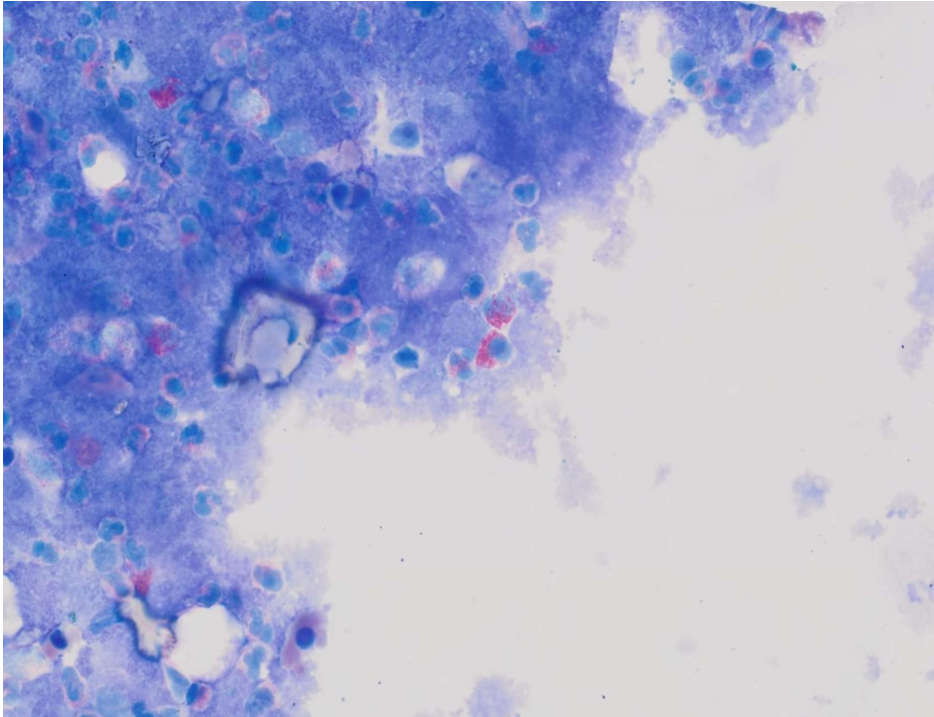

Correct responses are defined as those reflecting agreement among 80% or more of all participants or referees. Unacceptable responses are indicated by "\*\*\*\*\*" on the Flagging line of each specimen.